



Digital Pressure and Temperature Sensor



Introduction

Stevens Smart PT is an advanced digital pressure and temperature sensor ideal for water level measurements as well as many other types of pressure and fluid level monitoring applications. The SDI-12 communications interface provides universal compatibility with industry standard data loggers.

In addition to simple instantaneous pressure, level, and temperature measurements, Smart PT includes the ability to automatically record peak crest levels, calculate average level as well as standard deviation all without complex datalogger configurations. Other advanced features include adjustable fluid density, automatic water temperature density compensation, and adjustable local gravity compensation.

An M14-1 threaded sensor head allows for easy mounting to pipes. An included threaded cap offers a loop hole which can be used to mount weights or pull the sensor through pipes or other small areas. The Smart PT is built to last for years in the field with fully sealed and potted components, a robust ceramic membrane, stainless-steel housing, and an industrial-quality cable.



Table of Contents

Introduction.....	1
Order numbers.....	3
Performance Characteristics.....	3
Environmental Conditions	3
Warranty	4
Installing the Smart PT probe.....	4
Wiring.....	4
Vent Tube.....	4
Ice	4
Packaging for calibration and repair	5
SDI-12 Commands and Responses	6
Command quick reference	6
Variation in the last digits of pressure readings	6
Basic SDI-12 Commands	6
Advanced SDI-12 Commands.....	9
Configuring pressure, depth, and temperature units	9
Configuring gravity compensation.....	10
Configuring density compensation	11
Configuring the Smart PT for top-of-casing or reference-relative measurements.....	11
Restoring the Smart PT to the default configuration	13
Using the Smart Sampling features and digital crest gage mode.....	14
Example configurations for average and daily maximum.....	14
Using Excel to extract timestamped crest values from a data set	15
Appendix A - Metadata Commands in SDI-12 version 1.4	16
Appendix B – Calculation of depth	16



Order numbers

Ordering Number	Range in bar	Water depth in meters	Water depth in feet	Overpressure in meters
vented				
51168-201	0.2	2	6.6	50
51168-202	0.4	4	13	60
51168-203	1	10	33	100
51168-204	2	20	66	150
51168-205	4	40	130	250
51168-206	10	100	330	400
51168-207	20	200	660	400
non-vented (note: non-vented depth specs are assumed at sea level. Actual max depth depends on elevation and atmospheric pressure.)				
51168-303	1.4	4	13	90
51168-304	2	10	33	140
51168-305	4	30	100	240
51168-306	10	90	300	390
51168-307	20	190	630	390
32142	Recommended Yearly Calibration			

Performance Characteristics

Parameter	Unit
Pressure accuracy	0.1% Full scale
Long term stability	max 0.15% per year Full scale
Temperature accuracy	±0.25 °C
Average current consumption, SDI-12	0.9 mA
Average current consumption, Modbus	1.5 mA

Environmental Conditions

Parameter	Min	Max	Unit
Supply voltage during operation	6	18	V
Temperature during operation	-20	80	°C



Warranty

The Smart PT has internal surge protection components for lightning protection. However, damage due to lightning is not covered under the warranty.

Except for the 0.2 bar vented sensor, the Smart PT is warrantied to withstand freezing conditions without damage if the black cap is removed. The 0.2 bar vented sensor is more sensitive to overpressure and isn't warrantied for freezing conditions.

Installing the Smart PT probe

Wiring

Wire Color	Signal
Black	Ground
Red	+12Vdc
Blue	SDI-12 Data
White	RS485+ / B
Green	RS485- / A

Note: RS485 is used for firmware updates and future interface expansion.

Vent Tube

The vented version of the Smart PT has a tube running the length of the cable. This allows the water pressure on the front of the transducer to reference against barometric pressure.

The Smart PT ships with a black cap over end of the vent tube to prevent moisture ingress, and with a separate desiccant capsule. Before installation the dessicant capsule needs to be connected and the yellow cap removed.



Ice

The Smart PT ships with an engineered resin cap designed to protect the ceramic membrane. It's important to remove the cap if the Smart PT is expected to freeze. If the cap isn't removed, expanding ice trapped under the cap will damage the ceramic membrane.



Packaging for calibration and repair

To correct for long term drift, the Smart PT should be calibrated every year.

Before returning the sensor for calibration or repair, navigate to the 'Support' page at <http://www.stevenswater.com/> and fill out the RMA form.

If the sensor was used in contaminated water, the sensor must be cleaned before shipping. Coil and zip-tie the sensor cable before shipping.



SDI-12 Commands and Responses

Command quick reference

M: pressure, temperature M1: minimum, maximum M2: average, standard deviation

Variation in the last digits of pressure readings

Smart PT reports pressure results to a precision of 0.0001 bars or better. This ensures that each pressure range of the Smart PT will return results with the same number of significant figures. Because this level of precision is higher than either the accuracy or the inter-reading stability of the Smart PT, it's normal to see variation in the last few digits of the pressure reading.

Basic SDI-12 Commands

Command	Response	Description
a!	a<CR><LF>	Acknowledge active a – sensor address
aI!	a14ccccccmmmmmvvvxxx...xx<CR><LF> Example: Vented: 014STEVENSW_SVP01_VT_1234567890 Non-vented: 014STEVENSW_SVP01_NV_1234567890	Send identification a – sensor address 14 – SDI-12 protocol version ccc... – manufacturer identification mmm... – sensor identification vvv – sensor version xxx... – serial number
aAb	b<CR><LF> Example: b	Change address b – new address
?!	a<CR><LF> Example: a	Address query a – sensor address
aM!	atttn<CR><LF> Example: a0002	Request a single pressure and temperature reading t - seconds until the measurement is ready (always zero) n – number of data fields in the measurement (always two for this command)



Command	Response	Description
aD0!	a<value1><value2><CR><LF> Example: a+1.0+25.6	Send a single pressure and temperature reading a – sensor address value1 – depth or pressure value2 – temperature
aM1!	atttn<CR><LF> Example: a0004	Request min and max (crest and trough) since the last M1 command. Smart PT takes a sample every second and stores min and max in nonvolatile memory. Min and max are reset when the M1 command is received.
aD0!	a<min><max><tmin><tmax><CR><LF> Example: a+1.0+1.4+48+67	Send min and max since the last M1 command a – sensor address min – lowest pressure encountered since last M1 reading max – highest pressure encountered since last M1 reading tmin – seconds elapsed since the minimum reported in <min> tmax – seconds elapsed since the maximum reported in <max> See the section, “Using Excel to extract timestamped crest values from a data set” for more information on using tmin and tmax
aM2!	atttn<CR><LF> Example: a0003	Request average and standard deviation of pressure since the last M2 command Smart PT takes a sample every second and maintains a cumulative average and standard deviation. Average and standard deviation are reset when the M2 command is received.



Command	Response	Description
aD0!	a<avg><stddev><nsamples><CR><LF> Example: a+1.2+0.01+129	Send average and standard deviation since the last M2 command a – sensor address avg – average of all pressure samples taken since the last M2 reading stddev – standard deviation of all pressure samples taken since the last M2 reading nsamples – number of samples taken since the last M2 reading



Advanced SDI-12 Commands

Configuring pressure, depth, and temperature units

The Smart PT can be configured to report in various units of pressure and temperature.

To compensate for the density-temperature curve in water, the Smart PT Sensor uses Kell's formulation, as described in the publication *ITS-90 Density of Water Formulation for Volumetric Standards Calibration (Jones 1992)*. This, and the gravity parameter, are applied to all measurements returned in units of depth.

When the Smart PT is configured to report in units of pressure, rather than depth, no temperature compensation will be applied.

The non-vented Smart PT only reports in units of pressure. Because it measures the weight of the water column plus the atmosphere, it wouldn't be useful to report units of depth.

Command	Response	Description																				
aXR_PUNITS!	aPUNITS='UUU'<CR><LF> Example: aXR_PUNITS! aPUNITS='M'	Query pressure units UUU... – pressure units																				
aXW_PUNITS_UUU!	aPUNITS='UUU'<CR><LF> Example: aXW_PUNITS_M! aPUNITS='M'	Configure pressure units uuu... – pressure units <table><tr><td>* meters</td><td>M</td></tr><tr><td>* centimeters</td><td>CM</td></tr><tr><td>* millimeters</td><td>MM</td></tr><tr><td>* feet</td><td>FT</td></tr><tr><td>* inches</td><td>IN</td></tr><tr><td>bars</td><td>BAR</td></tr><tr><td>millibars</td><td>MBAR</td></tr><tr><td>kilopascals</td><td>KPA</td></tr><tr><td>pounds per square inch</td><td>PSI</td></tr><tr><td>default</td><td>BAR</td></tr></table> * Only allowed for vented	* meters	M	* centimeters	CM	* millimeters	MM	* feet	FT	* inches	IN	bars	BAR	millibars	MBAR	kilopascals	KPA	pounds per square inch	PSI	default	BAR
* meters	M																					
* centimeters	CM																					
* millimeters	MM																					
* feet	FT																					
* inches	IN																					
bars	BAR																					
millibars	MBAR																					
kilopascals	KPA																					
pounds per square inch	PSI																					
default	BAR																					
aXR_TUNITS!	aTUNITS='UU'<CR><LF> Example: aXR_TUNITS! aTUNITS='DC'	Query temperature units UU... – temperature units																				
aXW_TUNITS_UU!	aTUNITS='UU'<CR><LF> aXW_TUNITS_DC! aTUNITS='DC'	Configure temperature units <table><tr><td>degrees centigrade</td><td>DC</td></tr><tr><td>degrees fahrenheit</td><td>DF</td></tr><tr><td>kelvin</td><td>DK</td></tr><tr><td>default</td><td>DC</td></tr></table>	degrees centigrade	DC	degrees fahrenheit	DF	kelvin	DK	default	DC												
degrees centigrade	DC																					
degrees fahrenheit	DF																					
kelvin	DK																					
default	DC																					



Configuring gravity compensation

Gravity on the surface of the earth can vary by 0.7%, from a minimum of 9.7639 m/s² in Peru, to a peak of 9.8337 m/s² on the surface of the arctic ocean.

The Smart PT can be configured to compensate for local gravitational acceleration.

Wolfram Alpha provides a convenient tool to find your local gravitational acceleration:

<https://www.wolframalpha.com/input/?i=gravity+portland+oregon>

When the Smart PT is configured to report in units of pressure, rather than depth, no gravity compensation will be applied.

Command	Response	Description
aXR_GRAVITY!	aGRAVITY='vvv' <CR><LF> Example: aXR_GRAVITY! aGRAVITY='9.80665'	Query gravity a – sensor address vvv... – gravitational acceleration
aXW_GRAVITY_vvv!	aGRAVITY='vvv' Example: aXW_GRAVITY_9.80665! aGRAVITY='9.80665'	Configure gravity a – sensor address vvv... – gravitational acceleration Default: 9.80665 m/s ²



Configuring density compensation

The density of water can vary due to salinity, aeration, or suspended sediment.

The Smart PT can be configured to compensate for working fluid density.

Because the built-in temperature density curve is only valid for fresh water, temperature compensation will be disabled when the density parameter is modified.

Command	Response	Description
aXR_DENSITY!	aDENSITY='vvv' <CR><LF> Example: aXR_DENSITY! aDENSITY='1'	Query density a – sensor address vvv... – density
aXW_DENSITY_vvv!	aDENSITY='vvv' Example: aXW_DENSITY_1.1! aDENSITY='1.1'	Configure density a – sensor address vvv... – density Default: 1 g/mL


Configuring the Smart PT for top-of-casing or reference-relative measurements

The Smart PT can be configured to report depth measurements from actual or surveyed top of casing. Following this command table is an example.

Command	Response	Description
aXR_TOC_vvv!	aTOC='vvv' <CR><LF>	Query top of casing
aXW_TOC_vvv!	aTOC='vvv' Example: aXW_TOC_1! aTOC='1'	If non-zero, depth will be subtracted from the TOC value. See the section, "Calculation of depth with corrections" Default: 0
aXR_OFFSET_vvv!	aOFFSET='vvv' <CR><LF>	Query offset
aXW_OFFSET_vvv!	aOFFSET='vvv' Example: aXW_OFFSET_1! aOFFSET='1'	This value will be added to depth after all other corrections have been applied. See the section, "Calculation of depth with corrections" Default: 0



In this example, a Smart PT is installed in a 100 foot borewell, 75 feet from the top of casing. The bottom of the well is 10 feet below sea level.

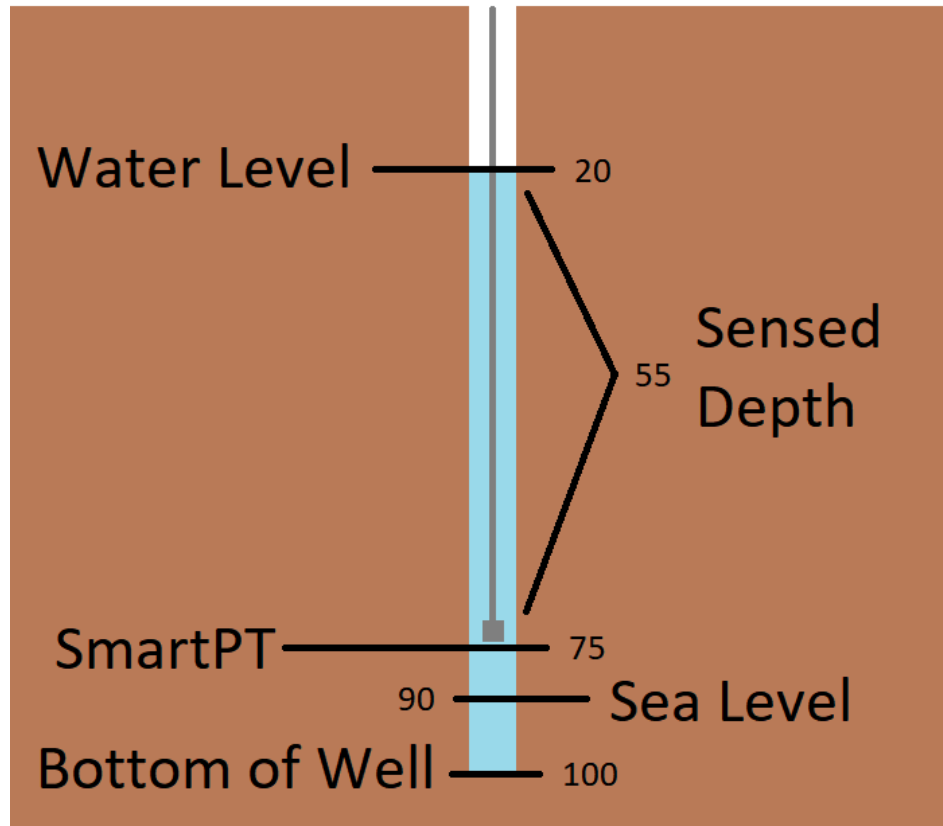

Without any special configuration the Smart PT will report the sensed depth, 55 feet.

To report feet above sea level, set the "offset" parameter to 15. The Smart PT will report the sensed depth plus the offset, for a reported value of 70.

`aXW_OFFSET_15!`

To report distance from water to top of casing, set "toc" to 75. The Smart PT will return the "TOC" value minus sensed depth, for a reported value of 20.

`aXW_TOC_75!`

To report distance from the water surface to bottom of well, set "offset" to 25. The Smart PT will return the sensed depth plus the offset, for a reported value of 80.

`aXW_OFFSET_25!`



Restoring the Smart PT to the default configuration


It may be useful to restore the Smart PT to the factory default configuration.

Command	Response	Description
aXD_*	arestore factory configuration...	Restore the sensor to a factory default state. Stored data will be lost. Sensor retains factory calibration.



Using the Smart Sampling features and digital crest gage mode

A conventional pressure sensor only samples data when requested by the logger. As seen in the chart below, if the sampling interval is set too long, there's a risk of missing critical events.

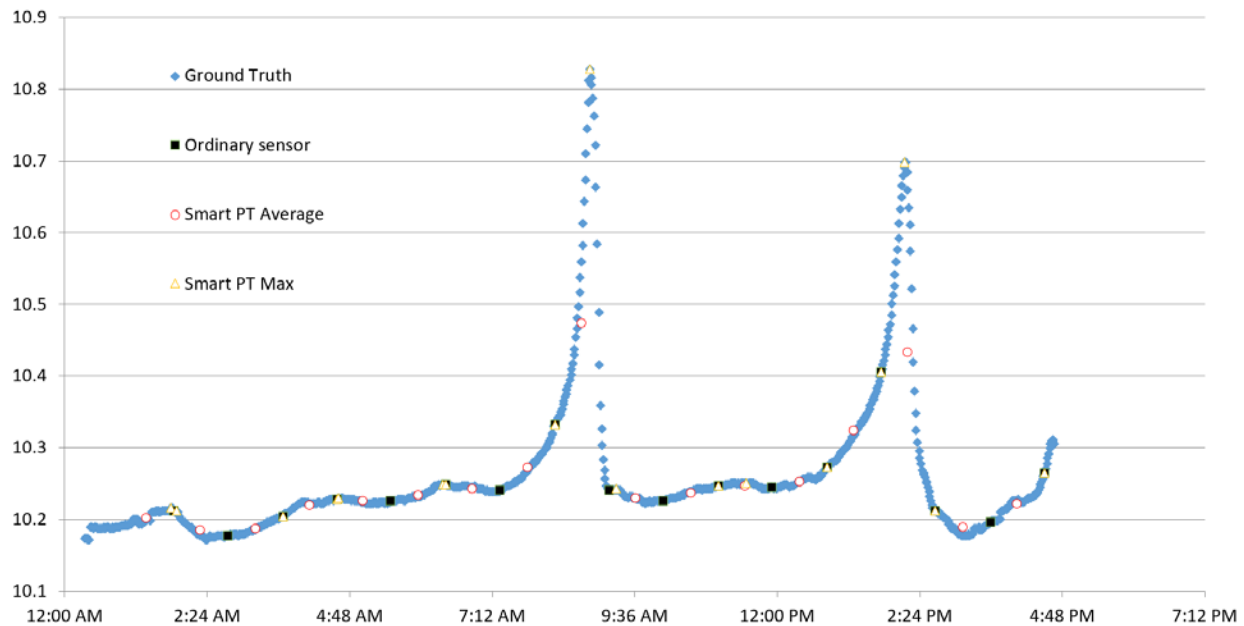

The Smart PT takes a sample once per second and can report relevant statistics on demand, including crest events. As you can see in the chart above, the Smart PT was able to accurately capture crest events that a conventional sensor would have missed.

The Smart PT is also able to report average and standard deviation over the logging interval. This may be useful for integrating data from rough water and quantifying surface roughness. Instead of a sliding window, the Smart PT uses a numerically stable online variance algorithm (Welford 1962) to maintain the mean and standard deviation since the last time those values were queried.

Example configurations for average and daily maximum

To record the ten-minute average, configure the data logger to sample the M2 command once every ten minutes.

To record the daily maximum, configure the data logger to sample the M1 command once every 24 hours.

Minimum and maximum values are backed-up to flash and will persist if the sensor loses power.



Using Excel to extract timestamped crest values from a data set

The Smart PT reports the time at which a min or max event occurred in the 3rd and 4th fields of the M1 response.

These values, tMin and tMax, show how many seconds ago the event occurred.

In the example below, a crest event occurred at 8:24:20 AM. The sensor was polled by a datalogger at 8:30:00 AM, at which time the sensor reported the crest event as happening 340 seconds in the past.

Logger timestamp	Min	Max	tMin	tMax		Time of crest	
						<u>A3-TIME(0,0,E3)</u>	
<u>8:30:00 AM</u>	1004	4996	33	<u>340</u>		<u>8:24:20 AM</u>	
8:40:00 AM	1004	4995	23	324		8:34:36 AM	
8:50:00 AM	1003	4999	47	310		8:44:50 AM	
9:00:00 AM	1001	4991	16	339		8:54:21 AM	



Appendix A - Metadata Commands in SDI-12 version 1.4

Revision 1.4 of the SDI-12 specification, released in May of 2017, adds a set of commands to access metadata – descriptions of the returned data including SHEF codes and units. The Smart PT sensor implements the 1.4 specification.

```
aIM0!                                a00002
aIM0_001!                            0,PW,BAR,pressure;
aIM0_002!                            0,TW,DC,temperature;
```

Appendix B – Calculation of depth

Depth is computed as follows

$$\text{depth} = \text{depth} * (9.80665 / \text{gravity}) * (1000 / \text{density})$$

If density is set to 1, the Smart PT will apply a temperature correction:

$$\text{density} = (999.83952 + 16.945176 * t - .0079870401 * t * t - 0.000046170461 * t * t * t + 0.00000010556302 * t * t * t * t - 0.0000000008054253 * t * t * t * t * t) / (1 + .016897850 * t);$$

If density is set to a value other than 1, that value will override the temperature correction.

If top of casing is greater than zero, depth is subtracted from top of casing:

$$\text{depth} = \text{top of casing} - \text{depth}$$

Finally, offset is added to the depth value:

$$\text{depth} = \text{depth} + \text{offset}$$
